



Title:

Certificate of Analysis (CoA)

Date: 5/7/2026
Date Tested: 5/14/2026
Customer: Peptides Optimized LLC
Testing material: Tesamorelin
Lot Number: TN2611
BT Sample ID: 005000039451403
Labeled Peptide Content/Potency: 10 mg
Storage: R.T.
Visual Description: Small clear vial: white sample, pink label, silver crimp, black plastic cap.
Labeled as: Tesamorelin
Manufacturer: N/A
Testing Purpose: FTIR and HPLC analysis for the identification, purity, potency and composition of a peptide product. It does not provide information on particulate matter, microbial contamination or presence of endotoxins.



Test	Method	Specification	Result
General Appearance	USP <630>	white powder	white powder
Mass	USP <41>	As recorded	104.5 mg
FTIR Identification and Composition Analysis	USP <197A>	Sample spectrum should confirm the content of peptide via characteristic bands	FTIR sample spectrum confirms the presence of Tesamorelin with addition of excipient(s)/fillers.
HPLC Purity of Peptide Assay	USP <621>	Specifications: $\geq 98\%$	99.7 %
HPLC Potency Assay	USP <621>	Specifications: 90 – 110% of 10 mg	12 mg (119.7 %)
Peptide-to-Excipients Ratio	USP <1151>	Recommended ratios of (1:2) to (1:10) for (peptide: excipients)	12 : 92.5 mg (1:7.7)


The results of the CoA relate only to the item(s) tested and applied to the sample as received.

Title:


Certificate of Analysis (CoA)



FTIR ID and Composition Analysis: Tesamorelin Lot TN2611

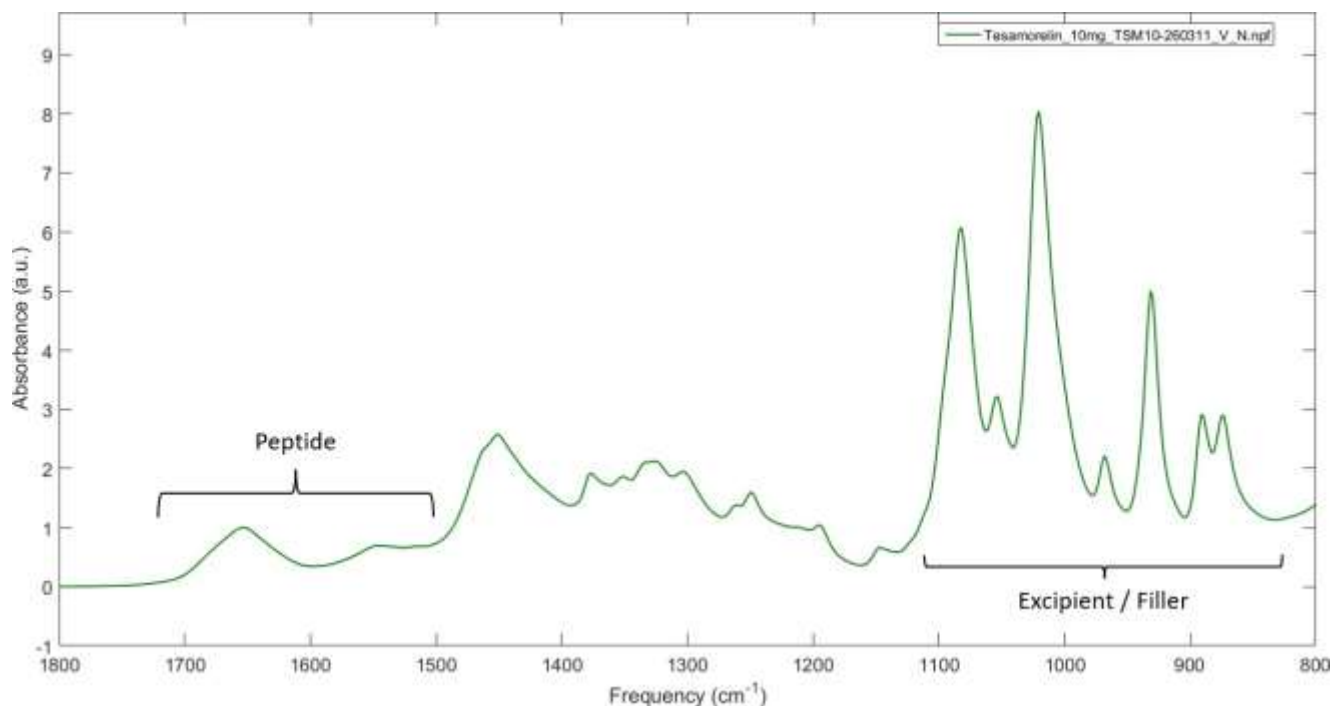

HPLC Purity and Potency Assay @ 280 nm: Tesamorelin Lot TN2611

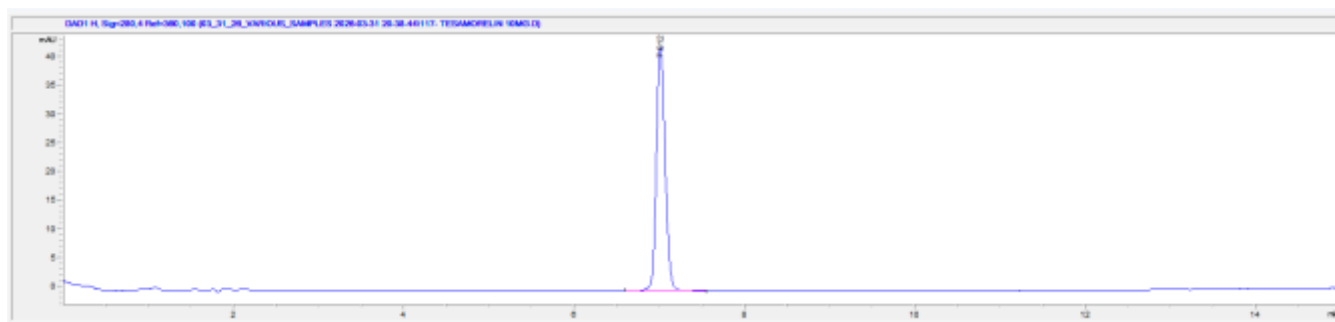

Tesamorelin Lot TN2611@ 280 nm

Peak #:	Retention Time (min)	Area (mAU*s)
1	7.012	303.4



COA #:
1556116

Page 3 of 3



Title:

Certificate of Analysis (CoA)

Test	Method	Specification	Result
Bacterial Endotoxins Test	USP <85>	40 EU/vial reconstituted	PASS

The results of the CoA relate only to the item(s) tested and applied to the sample as received.

Bacterial Endotoxins Test Tesamorelin Lot TN2611

Sample ID	Description	Volume (mL)	Endotoxin Limit (EU/vial)	Lysate Sensitivity (λ , EU/mL)	Result
TN2611	Tesamorelin	3	40 EU/vial	0.25	9.6 EU/vial

The sample passed a valid gel clot endotoxin test based on the type, mode of administration and dosage.